




# Disposable Respirator Fitting Instructions




- Users must follow instructions each time respirator is worn.
- It's the wearer's responsibility to obtain a proper fit.
- To choose the correct model/size Moldex Respirator you must fit test and user seal check.
- If you cannot obtain a proper fit do not enter the contaminated area.
- OSHA regulation 29 CFR 1910.134 (f) requires that the user must be fit tested before being assigned a respirator and annually thereafter.**
- Use an appropriate OSHA (or other official regulatory agency) approved fit test method.
- User must be clean-shaven. Any facial hair, such as beards or long sideburns, may prevent the respirator from fitting properly.
- Re-fit test when there are any changes to the wearers physical condition that may affect fit and/or when changing from any model/size to another respirator.

## 2-STRAP DISPOSABLE RESPIRATORS



- Hold respirator in hand with molded nose contour (narrow end) at finger tips, allowing headstraps to fall below hand (Fig 1).
- Place respirator under chin with molded nose contour (narrow end) up. Nose cushion must not be creased inside respirator. Raise top strap to top back of head. Pull shorter bottom strap over head, below ears, to around neck. **Do not wear with only one strap because it may affect fit.** (Fig 2).
- Adjust respirator for comfortable fit (Fig 3).
- Each time user enters contaminated area seal should be fit checked. Cover front of respirator by cupping both hands. **INHALE SHARPLY.** A negative pressure should be felt inside respirator. If any leakage is detected at respirator edges, adjust straps by pulling back along the sides and/or reposition respirator. Repeat until sealed properly, otherwise see your supervisor. Entry into a contaminated area with an improper fit may result in sickness or death (Fig 4).

## SMARTSTRAP® RESPIRATORS

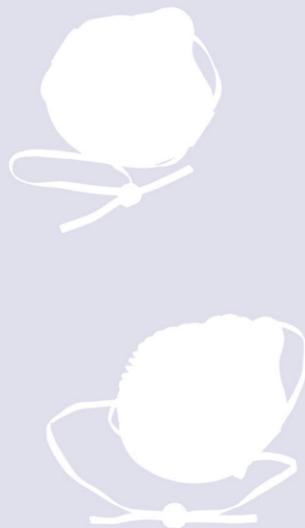

- Pull adjustment clip and strap fully below the bottom of the mask (Fig 1).
- Place strap around neck so outside of shell is against chest (Fig 2).
- a) Fit mask to face and pull top of strap to crown of head. Nose cushion or foam cushion must be uncreased inside of respirator. b) Always use both top and bottom straps (Fig 3).
- To tighten pull both strap tabs (Fig 4). To loosen, grasp both sides of neck strap and pull.
- Each time user enters contaminated area respirator must be seal checked. Cover front of respirator by cupping both hands. (Fig 5). **INHALE SHARPLY.** A negative pressure should be felt inside respirator. If any leakage is detected at respirator edges, tighten or adjust strap by pulling back along the sides and/or reposition respirator. Repeat until sealed properly, otherwise see your supervisor. Entry into a contaminated area with an improper fit may result in sickness or death.
- To hang around neck, pull top strap away from head, then pull mask down (Fig 2).

## HANDYSTRAP® RESPIRATORS



- Attach buckle behind neck with shell against chest.
- a) Fit mask to face and pull top of strap to crown of head. Nose cushion must be uncreased inside respirator. b) Always use top and bottom part of strap. Adjust tension for a comfortable fit. When changing from any model/size to another respirator, you must fit test.
- Each time user enters contaminated area respirator must be seal checked. Cover front of respirator by cupping both hands. **INHALE SHARPLY.** A negative pressure should be felt inside respirator. If any leakage is detected at respirator edges, adjust strap by pulling back along the sides and/or reposition respirator. Repeat until sealed properly, otherwise see your supervisor. Entry into a contaminated area with an improper fit may result in sickness or death.
- To hang around neck:
  - Undo buckle.
  - Allow strap to fall around neck.
  - Pull mask down to chest.
 OR
  - Pull top strap forward away from head.
  - Adjust tension to allow mask to hang freely.

# MOLDEX®

**U.S. & CANADA**  
10111 JEFFERSON BOULEVARD  
CULVER CITY, CA 90232  
TEL: +1 (310) 837-6500 EXT. 550  
FAX: +1 (310) 837-9563  
sales@moldex.com  
www.moldex.com

**BRAZIL**  
AVENIDA IPIRANGA, 104-22  
ANDAR, SÃO PAULO,  
SP CEP:01046-010  
BRASIL  
FONE/FAX: 113255-0555  
CEL: +55-11-99486-4083  
moldexbrazil@moldex.com  
moldex.com/pt-br

**AUSTRALIA**  
P.O. BOX 4086  
CARLINGFORD NORTH, NSW 2118  
TEL: 1300 MOLDEX (1 300 665 339)  
moldexaustralia@moldex.com  
moldex.com/au

**NEW ZEALAND**  
3 SPENCE ROAD  
HENDERSON, AUCKLAND, NZ  
TEL: +64 027 243 1244  
moldexnz@moldex.com  
moldex.com/nz

**MOLDEX JAPAN K.K.**  
FIS BLDG, 403  
SHIMOMARUYA-CHO,  
NAKAGYO-KU, KYOTO, 604-8006  
JAPAN  
TEL: 011-81757785070  
FAX: 011-81752568657  
moldexjapan@moldex.com

### TECHNICAL HELP LINE

For technical assistance call Moldex Technical Service Department at 1 (310) 837-6500, ext. 512 or 1 (800) 421-0668, ext. 512 or email tech@moldex.com.

ATTENTION: If these respirators are used against any contaminants it must be used in accordance with the appropriate local, state and federal regulations including 29 CFR 1910.134 as a minimum.

Moldex® and the PVC-Free logo are registered trademarks of Moldex-Metric, Inc.



9900-037 REV C 11/24